Therapy System

Software Upgrade Instructions

Follow these procedures completely.

1. Check Current Unit Version Information

Refer to the Therapy System User Manual for instructions of how to check the Unit Version Information. Record the current S/W Versions for reference.

2. Turn Therapy System On

Position Mains Power Switch in the On position.

3. Insert Software Upgrade

Remove the MMC Card from the System and insert the Software Upgrade MMC Card into the System MMC Port. See Figure 1.

Figure 1

4. Access Upgrade Screen

Simultaneously press the Stop, Pause, and Start Buttons. See Figure 2.

Figure 2

5. Upgrade Control Board

If upgrading from **Software Version 3.7 or earlier**, the screen in **Figure 3** will appear. Press the Upgrade Control S/W/ from MMC Button. Once the Upgrade is complete, the system will automatically reboot and return to the Home Screen. Proceed to Step 6 and continue through Step 8.

If upgrading from **Software Version 3.8 or later**, the screen in **Figure 5** will appear. Disregard Step 6 and follow Steps 7 and 8.

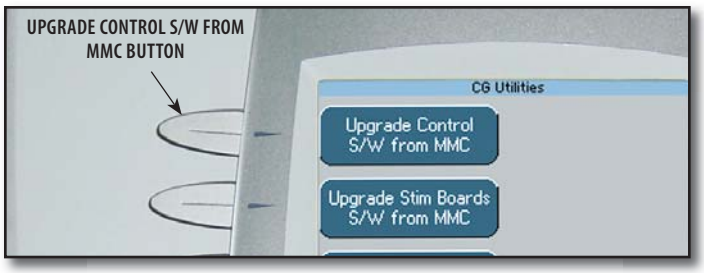

Figure 3

6. Access Software Upgrade Screen

Simultaneously press the Stop, Pause, and Start Buttons. See Figure 4.

Figure 4

7. Upgrade Software from MMC

Press the Upgrade Software from MMC Button. See Figure 5. Once the Upgrade is complete, the system will automatically reboot and return to the Home Screen.

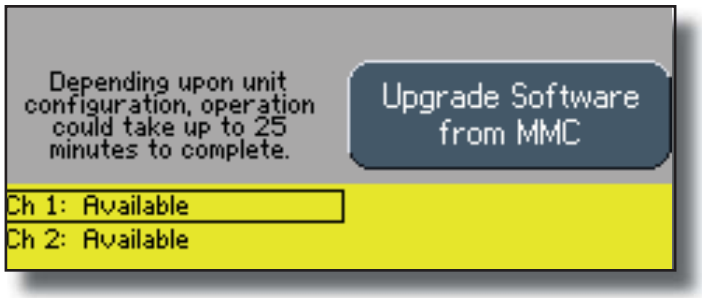
Depending upon unit configuration, operation could take up to 25 minutes to complete.
Upgrade Software from MMC
Ch 1: Available
Ch 2: Available

Figure 5

8. Remove Software Upgrade MMC

After all software is upgraded, remove the Software MMC and re-install the Therapy System MMC.

Reset Therapy System by turning the Mains Switch Off and back On.

CHATTANOOGA GROUP
ISO 13485 CERTIFIED
CE 0413
4717 Adams Road
P.O. Box 489
Hixson, TN 37343 U.S.A.
1-423-870-2281
1-800-592-7329 U.S.A.
1-800-361-6661 CANADA
+1-423-870-7200 OUTSIDE U.S.A.
+1 423-870-2046 OUTSIDE U.S.A. FAX
chattgroup.com

27832E
© 2008 Encore Medical, L.P.